

Interactive comment on “TECHNICAL NOTE: Coupling infrared gas analysis and cavity ring down spectroscopy for autonomous, high temporal resolution measurements of DIC and $\delta^{13}\text{C}$ -DIC” by Call et al.

Mitchell Call et al.

m.call.10@student.scu.edu.au

We thank both referees for their positive and constructive reviews which have helped improve our manuscript. We have revised the manuscript with the changes outlined in the following.

General comments by Anonymous Referee # 1

The brief technical note by Call et al. presents an interesting case of coupling two commercially available instruments for combined analysis of [DIC] and $\delta^{13}\text{C}$ -DIC analysis that may have a wide range of applications under both lab and field conditions. This team has been very active in these novel applications and the technical aspects of the study appear to be very sound and the intercalibration with IRMS measurements is promising. I also welcome the fact that the authors made ample technical information and scripts available for those who wish to implement this approach. My main concern is their interpretation of the data resulting from the 8-day incubation experiments which is used as an example application. The Keeling approach used is in my opinion not appropriate to apply to this dataset since it is only applicable to period where only respiration occurs: then you have a situation where a 2-source mixing model applies. During periods of illumination, when primary production is important, this principle does not hold and applying a Keeling approach is not valid, what is happening here is a case of isotope fractionation, not isotope mixing.

The authors should thus only apply the Keeling approach to ‘nighttime’ data. Also, more information should be added on how the Keeling method was applied, i.e. what type of regressions were used. There is a wealth of literature on the importance of using a correct regression method, Pataki et al. (2003) and Zobitz et al (2006) are a good start:

Zobitz JM, Keener JP, Schnyder H, & Bowling DR (2006) Sensitivity analysis and quantification of uncertainty for isotopic mixing relationships in carbon cycle research. *Agricultural and Forest Meteorology* 136: 56-75

Pataki, D.E., Ehleringer, J.R., Flanagan, L.B.D.Y., Bowling, D.R., Still, C.J., Buchmann, N., Kaplan, J.O., Berry, J., 2003b. The application and interpretation of Keeling plots in terrestrial carbon cycle research. *Global Biogeochem. Cycles* 17 (1), 1022, doi:10.1029/2001GB001850

Whilst Keeling plots have been applied to periods when CO_2 sources (respiration) and sinks (primary production) occur simultaneously, that is, during periods of illumination (Vardag et

al., 2016), we believe a discussion on the validity of this approach is beyond the scope of this technical note. Thus, we have amended the manuscript such that the Keeling approach was applied only to ‘nighttime’ periods, i.e. when only respiration occurs and the DIC isotope signal is purely a function of mixing.

With regards to the type of regression selected, the original manuscript did state that that a model II regression was used (L33, P7). Again, we believe that detailing the specific aspects of the regression models available is beyond the scope of this technical note, however, we have now referenced the review by Pataki et al. (2003) and provided additional detail:

“Keeling plots (Keeling, 1958) visualize a simple two component mixing model and are commonly used to interpret sources of added carbon in aquatic, terrestrial and atmospheric sciences (see (Pataki et al., 2003) for details on underlying assumptions and types of regression models available). Using a Model II regression (which assumes errors in the measurement of both variables), the y-intercept of the regression between the inverse of DIC concentration (1/DIC) and $\delta^{13}\text{C}$ -DIC estimates the isotopic composition of the carbon source. The approach has been used to determine the isotopic composition of the DIC source in various settings including freshwater lakes (Karlsson et al., 2007), coral reefs (Carvalho et al. 2015), mangroves (Maher et al., 2013a) and groundwaters (Porowska, 2015).”

Minor suggestions from Anonymous Reviewer # 1:

-3: why is ‘instrument air’ needed or used, and not a CO₂-free carrier gas? Would this not simplify and improve measurements, or is there a reason I’m overlooking that a certain background level of CO₂ is required? If not, you could simply strip out the CO₂ with either a cold trap or a CO₂ scrubber.

Briefly, to achieve the precision and accuracy obtained by the AIRICA-CRDS based on the CO₂ extracted from a small sample (2 ml), we used a gas stream with a background level of CO₂. This allowed for a greater proportion of the integration period to be within the manufacturer specifications (380 ppm is the minimum concentration for the guaranteed precision of the CRDS instrument by the manufacturer). Thus, a mass balance was required to account for the $\delta^{13}\text{C}$ value of the carrier gas to determine a $\delta^{13}\text{C}$ -DIC. This is now explained in greater detail throughout the manuscript.

The decision to use instrument air (as opposed to CO₂-free carrier gas) was first outlined at P3 L10-15: *“The carrier gas used comprised of instrument air, with a background CO₂ mixing ratio of 289 ppm and a $\delta^{13}\text{C}$ -CO₂ of -10.1 ‰. This carrier gas was used as the CRDS requires a gas with a similar composition to air. Furthermore, as the lower specified concentration range of the CRDS is ~ 380 ppm, the background CO₂ enables accurate measurement of a $\delta^{13}\text{C}$ -CO₂ over a greater proportion of the integration period...”*

We acknowledge that both Reviewer’s had similar comments as to why instrument air was used. Therefore, we have provided additional detail in the aforementioned text to clarify the use of a CO₂-free carrier gas earlier in the manuscript:

“The carrier gas used comprised of instrument air (as opposed to CO₂-free carrier gas), with a background CO₂ mixing ratio of 289 ppm and a $\delta^{13}\text{C}$ -CO₂ of -10.1 ‰. This carrier gas was used as the CRDS requires a gas with a similar composition to air. Furthermore, as the lower specified concentration range of the CRDS is ~ 380 ppm, to achieve the precision and

accuracy obtained by the AIRICA-CRDS from the CO₂ extracted from a small sample (2 ml), the background CO₂ enables accurate measurement of a δ¹³C-CO₂ over a greater proportion of the integration period (discussed below)."

-p5: explain in more detail how the standards were prepared – preparing these requires some precautions in terms of removing all dissolved CO₂ prior to dissolving your powdered standards etc.

Standards were made by dissolving carbonate solids in ultra-pure water (18.2 Milli-Q®) which had a DIC concentration < 2 μmol kg⁻¹. We have added this sentence:

"All standards were made by dissolving carbonate solids in ultra-pure water (18.2 Milli-Q®)."

-p5: salinity has no units, remove 'ppt'

We have removed 'ppt' in the revised manuscript.

-p7 and further throughout the ms: use correct terminology when referring to higher or lower d13C values, e.g. L19: 'depleted d13C-DIC' should be 'lowered d13C-DIC', L23: 'enriching d13C-DIC values' should be 'increasing d13C-DIC values', L27: 'enrichment of d13C-DIC' should be 'increase of d13C-DIC' etc.

We have made these changes throughout the manuscript.

-p8: see initial comments on Keeling plot approach: (i) provide details on regression techniques, and (ii) should not be applied on data from periods with primary production.

Please refer to our aforementioned response to the initial comments.

-p8 L21: ulva ! Ulva sp. (capital, italics)

We have made this change in the revised manuscript.

-p8 L22 : use one decimal only for d13C data

We have made this change in the revised manuscript.

References used in this reply:

Martz, T. R., Daly, K. L., Byrne, R. H., Stillman, J. H., and Turk, D.: Technology for ocean acidification research: Needs and availability, *Oceanography*, 28, 40-47, 10.5670/oceanog.2015.30, 2015.
Pataki, D. E., Ehleringer, J. R., Flanagan, L. B., Yakir, D., Bowling, D. R., Still, C. J., Buchmann, N., Kaplan, J. O., and Berry, J. A.: The application and interpretation of Keeling plots in terrestrial carbon cycle research, *Global Biogeochemical Cycles*, 17, n/a-n/a, 10.1029/2001GB001850, 2003.
Vardag, S. N., Hammer, S., and Levin, I.: Evaluation of 4 years of continuous δ¹³C(CO₂) data using a moving Keeling plot method, *Biogeosciences*, 13, 4237-4251, 10.5194/bg-13-4237-2016, 2016.

General comments by Referee # 2, Neils Munksgaard

This article describes the analytical procedure and performance of two commercial instruments coupled to provide near-simultaneous, high quality data on DIC concentrations and DIC 12C/13C isotope ratios (delta 13C). Similar automated and high-frequency data have previously been obtained using custom designed instruments in both the laboratory and the field (as referenced). The merit of the approach described here is that the interfacing of

the two instruments, each optimised for their respective analysis, provides combined data with improved precision and accuracy compared to the previously described methods.

The authors convincingly demonstrate that the technique works well in the laboratory and comment that it may also be field deployable with adequate power and shelter. However, the practicalities of field deployment would not be easy as the several components (CRDS, AIRICA, LICOR, PC, monitor, air tank, power etc) must weigh 50-60 kg. Also, the authors describe their system as 'simple' which might be slightly 'optimistic', especially in a field setting. Further testing would be needed to demonstrate performance in the field (e.g. sensitivity to temperature changes).

In reviewing the technologies available to ocean acidification scientists, Martz et al. (2015) noted that the replication of a described customised system can be "either untenably time consuming or completely intractable". Our description of the simplicity of the AIRICA-CRDS refers to the fact that our new method does not require the need to design or replicate a customised system. We believe that coupling two high precision, commercially available instruments without any modification to their hardware does represent simplicity.

Our comments regarding the potential for field deployment is based on both instruments being used in field settings previously. We acknowledge that further testing would need to demonstrate its performance in the field and as such, have added:

"however, further testing is required to test this capability."

I find this a high quality technical note that reads very well and the procedures are mostly clearly described, it is also great that the supplement includes computer coding to aid other researchers setting up this technique.

I'm curious as to why 'zero air' (CO₂ free air) was not used as carrier – instead, air with a reduced CO₂ content was used requiring a mass balance calculation to derive the sample isotope results. I would think this potentially degrades performance.

Please refer to the response provided to Anonymous Referee #1's similar comment.

Regarding the previous comment (ref #1) on the use of the Keeling plot for the linear sections of Fig. 4 (discussion P 8 re respiration and photosynthetic fixation during the algae bloom experiment), I agree that this treatment seem valid for the dark sections (respiration) – here the two mixing components would be (1) the existing DIC pool and (2) the added DIC (respired CO₂ – although this could be a constant mixture of CO₂ coming from more than one source). For the light sections (photosynthesis), the 'mixing' line is in effect an 'un-mixing' line (CO₂ - and preferentially ¹²CO₂ – being removed from the DIC pool). How such a line should be interpreted seems highly uncertain given the associated (and uncertain/variable) isotopic fractionation effects. I suggest modifying this section of the discussion but an exhaustive explanation should not be necessary in this technical note.

Please refer to our response to Anonymous Referee #1.

Specific comments:

1. P3 line 12-14: need more specifics for the 'Dickson CRM', justify why CO₂ free air was not used

We have added specifics for the Dickson CRM to that sentence:

“(Batch # 136, DIC 2021.15 $\mu\text{mol kg}^{-1}$, Sal 33.678)”

2. P3 line 17: ‘CO₂ only operating mode’ is confusing here – is it because this instrument also can measure CH₄?

Yes, the CRDS (Picarro G2201-*i*) can also simultaneously measure the carbon stable isotope ratio of methane ($\delta^{13}\text{C-CH}_4$). We have added the following to the sentence:

“(the CRDS can also simultaneously determine the carbon stable isotope ratio of methane)”.

3. P5: May point out that blooming algae would have been present in the sampled seawater – is there any information on the type/species?

No, species type was not determined. This level of detail is beyond the scope of the manuscript.

4. P7 line 21: Similar systematic changes in DIC and d13C was previously described for coral by the Bass et al 2012 study.

We have included the following reference to this paper in the revised manuscript:

“Similar diel variations were observed for DIC and $\delta^{13}\text{C-DIC}$ in a mesocosm coral reef metabolism experiment (Bass et al., 2012).”

5. P8: For the algae bloom experiment, additional details are required on how the uncertainty of the intercept d13C values in the Keeling plots were derived (Fig. S2) – the uncertainties should be added to the figures.

We have updated Fig. S2 to include the uncertainties of both the slope and the intercept of the regression equation. Intercept uncertainty is based on the statistical uncertainty associated with the regression. The Model II regression (geometric mean regression) assumes significant errors in the measurement of both variables. Pataki et al. (2003) and references therein provides an explanation on the how the uncertainties are derived for this regression model and we have added this reference when discussing the intercept uncertainty.

6. P8 line 3: It should be emphasised that uncertainty of the intercept d13C value is very dependent on the range of [DIC] in each plot – and much higher than the uncertainty of the individual d13C DIC data points. Could this uncertainty be improved by manipulating carrier flow and sample size etc to increase the [DIC] range? Would using CO₂ free air as carrier increase the range?

The uncertainty of the intercept value is very dependent on the rate of change in DIC concentration during the incubation period i.e. the magnitude of the respiration signal. We have changed the manuscript to emphasise this:

“The uncertainty in the intercept (i.e. the $\delta^{13}\text{C-DIC}$ source value) is dependent on the rate of change in DIC concentration during the dark incubation period. Uncertainty decreased as the absolute change in DIC increased, achieving < 2 ‰ uncertainty when the change in DIC was greater than ~ 40 $\mu\text{mol kg}^{-1}$ (Fig. 5).”

We have also noted that the uncertainty of the intercept value is much higher than the uncertainty for each $\delta^{13}\text{C}$ -DIC and DIC data value used to determine the intercept value:

“It is noted that the intercept uncertainty is much higher than the uncertainty for each $\delta^{13}\text{C}$ -DIC and DIC value (± 0.14 ‰ and ± 1.5 to $2 \mu\text{mol kg}^{-1}$ respectively).”

The rate of change in DIC concentration is a function of the experimental conditions (in this case the respiration rate), thus, manipulating the individual features of the AIRICA-CRDS (e.g. carrier flow, sample size, etc.) would not improve the intercept uncertainty.

7. P8 line10: Suggest expanding this explanation a bit: initial source is terrestrial OM present in the sampled coastal seawater, then marine OM from the *Ulva* sp introduced later in the experiment

We have amended a later sentence to:

“Thus, results suggest a distinct shift in the source of DIC during the course of the experiment, from terrestrially derived OM present in the sampled coastal seawater to marine derived OM at the end. This is likely due to a shift towards a dominance of marine organic matter toward the end of the experiment as a result of the algal bloom and the added macroalgae (added on day 6, Fig. 4).”

8. Figure 3 shows a very good correlation between AIRICA-CRDS and IRMS results for samples, yet supplement Table S1 seems to show an offset of 0.3-0.5 ‰ between the two techniques

Accuracy of the AIRICA-CRDS $\delta^{13}\text{C}$ -DIC was determined by direct comparison with IRMS measurements collected simultaneously during the algal bloom experiment. Figure 3 shows these results.

Table S1 on the other hand shows results of the precision results. The table supplements the observed decreasing $\delta^{13}\text{C}$ -DIC uncertainty with higher DIC concentrations is shown in Fig. 2B. The purpose of this Table was to highlight the precision based on repeated measurements of standards made at differing concentrations, rather than a determination of accuracy.

9. Supplement Fig. S1: Seems surprising that rinse, DIC and $\delta^{13}\text{C}$ cycles produce same concentration (peak value) - is the concentration limited by settings of the AIRICA?

Pre-testing allowed careful adjustment of gas flow rates and sample injection rates to ensure concentrations peaks were similar for both analysis types, with peak concentrations falling in the optimal range for both the AIRICA and CRDS instruments.

TECHNICAL NOTE: Coupling infrared gas analysis and cavity ring down spectroscopy for autonomous, high temporal resolution measurements of DIC and $\delta^{13}\text{C}$ -DIC

Mitchell Call^{1,3}, Kai G. Schulz², Matheus C. Carvalho², Isaac R. Santos³ and Damien T. Maher^{1,3}

¹School of Environment, Science and Engineering, Southern Cross University, Lismore, NSW, 2480, Australia

²Centre for Coastal Biogeochemistry, School of Environment, Science and Engineering, Southern Cross University, Lismore, NSW, 2480, Australia

³National Marine Science Centre, School of Environment, Science and Engineering, Southern Cross University, Coffs Harbour, NSW, 2450, Australia

Correspondence to: Mitchell Call (m.call.10@student.scu.edu.au)

Abstract. A new approach to autonomously determine concentrations of dissolved inorganic carbon (DIC) and its carbon stable isotope ratio ($\delta^{13}\text{C}$ -DIC) at high temporal resolution is presented. The simple method requires no customised design. Instead it uses two commercially available instruments currently used in aquatic carbon research. An inorganic carbon analyser utilising non-dispersive infrared detection (NDIR) is coupled to a Cavity Ring-down Spectrometer (CRDS) to determine DIC and $\delta^{13}\text{C}$ -DIC based on the liberated CO_2 from acidified aliquots of water. Using a small sample volume of 2 ml, the precision and accuracy of the new method was comparable to standard isotope ratio mass spectrometry (IRMS) methods. The system achieved a sampling resolution of 16 mins, with a DIC precision of ± 1.5 to $2 \mu\text{mol kg}^{-1}$ and $\delta^{13}\text{C}$ -DIC precision of $\pm 0.14 \text{ ‰}$ for concentrations spanning 1000 to $3600 \mu\text{mol kg}^{-1}$. Accuracy of $0.1 \pm 0.06 \text{ ‰}$ based on DIC concentrations ranging from $2000 \mu\text{mol kg}^{-1}$ to $2230 \mu\text{mol kg}^{-1}$ was achieved during a laboratory-based algal bloom experiment. The high precision data that can be autonomously obtained by the system should enable complex carbonate system questions to be explored in aquatic sciences using high temporal resolution observations.

Keywords. Dissolved inorganic carbon (DIC), stable isotopes, carbonate chemistry, laser spectroscopy, keeling plot.

1 Introduction

Dissolved inorganic carbon (DIC) is an important component of the evolving global carbon cycle, with ~ 26 % of yearly anthropogenic carbon dioxide (CO_2) emissions stored as DIC in the global ocean (Le Quéré et al., 2015). This influx of carbon to the oceans has resulted in increased field-monitoring (Sabine et al., 2010), laboratory-based experiments of how changing seawater carbonate chemistry effects biological process (Gattuso and Hansson, 2011), as well as the development of new measurement technologies (Byrne, 2014; Martz et al., 2015). Currently, the spatial and temporal coverage of paired DIC and carbon stable isotope ratio ($\delta^{13}\text{C}$ -DIC) measurements is poor (Becker et al., 2016). However, greater interest is being placed on the coupled high-resolution measurement of DIC and $\delta^{13}\text{C}$ -DIC as it can provide insights into the processes controlling DIC concentrations, helping elucidate flows of carbon within and between reservoirs (Bass et al., 2014b).

Formatted: Header distance from edge: 1.25 cm,
Footer distance from edge: 1.25 cm

Whilst a variety of methods to autonomously measure DIC concentrations have been developed (Bandstra et al., 2006; Fassbender et al., 2015; Huang et al., 2015; Liu et al., 2013) the conventional method for determining $\delta^{13}\text{C}$ -DIC requires discrete samples to be collected and stored prior to acidification and analysis in a laboratory by isotope ratio mass spectrometry (IRMS). IRMS analysis offers high precision, however, the collection, handling and preservation of discrete samples may introduce sampling artefacts and reduce accuracy (Li and Liu, 2011; Taipale and Sonninen, 2009). Furthermore, the laborious process limits sampling frequency, resulting in low temporal and spatial coverage of coupled DIC and $\delta^{13}\text{C}$ -DIC measurements.

High resolution, field-based measurement of CO_2 and its carbon stable isotope value ($\delta^{13}\text{C}$ - CO_2) is now achievable via laser spectroscopy systems such as Cavity Ring-Down Spectrometers (CRDS) (Crosson, 2008) and Off-Axis Integrated Cavity Output Spectroscopy (OA-ICOS) (Baer et al., 2002), with precision and accuracy comparable to laboratory-based IRMS (Vogel et al., 2013; Berryman et al., 2011; Midwood and Millard, 2011). The use of CRDS in the aquatic environment is becoming more prevalent with CRDS successfully coupled to air-water equilibrators for on-site, high-resolution measurement of dissolved CO_2 and its isotopic composition (Maher et al., 2013b; Becker et al., 2012). Recently, Bass et al. (2012) coupled a CRDS to a customised acidification interface utilising expanded polytetrafluoroethylene (ePTFE) tubing to measure in-situ concentrations of DIC and its $\delta^{13}\text{C}$ -DIC. The permeable membrane based equilibration system autonomously measured DIC and $\delta^{13}\text{C}$ -DIC at 15 minute intervals to a precision of $\pm 10 \mu\text{mol kg}^{-1}$ and $\pm 0.2 \text{‰}$ respectively, and has been shown to be sufficient for identifying spatial and short-term temporal variability in DIC concentrations in a variety of aquatic systems (Bass et al., 2014a; Bass et al., 2014b; Bass et al., 2013). However, a precision of $\sim 2 \mu\text{mol kg}^{-1}$ or better is required in order to assess other processes such as long-term anthropogenic-induced changes to oceanic carbon chemistry (Newton et al., 2014) or in laboratory-based experiments when trying to detect small changes in DIC.

This paper presents an alternative approach to autonomously determine concentrations of DIC and $\delta^{13}\text{C}$ -DIC. The simple method does not require the need to design or replicate a customised system. Instead, it couples two commercially available instruments, an inorganic carbon analyser utilising non-dispersive infrared detection (NDIR) and a CRDS. The system can be automated, is low maintenance, and achieves a sampling resolution of ~ 16 mins. Using only a small sample volume (2 ml), the method achieves high precision and accuracy comparable to traditional IRMS techniques.

2 Materials and procedures

2.1 Approach

Two commercially available instruments, an Autonomous Infra Red Inorganic Carbon Analyser (AIRICA, Marianda Company, Kiel, Germany), and a CRDS (Picarro G2201-i, Picarro Inc., Santa Clara, CA, USA) were coupled to autonomously measure concentrations of DIC and its carbon stable isotope ratio ($\delta^{13}\text{C}$ -DIC) based on the CO_2 extracted from acidified samples (Fig. 1). These instruments offer high precision and accuracy, and are currently used in aquatic carbon research. To test the response of the method, here-in termed AIRICA-CRDS, laboratory-based experiments on precision were conducted as well as a mesocosm experiment simulating an algal bloom in coastal waters.

2.2 Instrumentation

The AIRICA system determines DIC to within ± 1.5 to $2 \mu\text{mol kg}^{-1}$ (0.1 %) based on the NDIR gas analysis method (Goyet and Snover, 1993; O'Sullivan and Millero, 1998). Briefly, the AIRICA's high precision syringe pump draws a sample into a stripper that is pre-loaded with acid, effectively reducing the sample pH below 4.5 and converting all DIC to CO_2 . A carrier gas strips the CO_2 from the acidified sample and the gas stream flows through a Peltier-element cooled condenser, followed by a Nafion dryer (both reducing water vapour content) before measurement by a NDIR analyser (LI-COR LI-7000, LI-COR Inc., Lincoln, NE, USA). DIC concentrations are determined by integrating the CO_2 mixing ratio signal in the NDIR analyser over the integration period, with the area versus concentration relationship established by 5-point calibration using in-house standards. The calibration factor was validated against Dickson certified reference materials (CRMs; [Batch # 136, DIC 2021.15 \$\mu\text{mol kg}^{-1}\$, Sal 33.678](#)). The carrier gas used comprised of instrument air ([as opposed to \$\text{CO}_2\$ -free carrier gas](#)), with a background CO_2 mixing ratio of 289 ppm and a $\delta^{13}\text{C-CO}_2$ of -10.1 ‰. This carrier gas was used as the CRDS requires a gas with a similar composition to air. Furthermore, as the lower specified concentration range of the CRDS is ~ 380 ppm, [to achieve the precision and accuracy obtained by the AIRICA-CRDS from the \$\text{CO}_2\$ extracted from a small sample \(2 ml\)](#), the background CO_2 enables accurate measurement of a $\delta^{13}\text{C-CO}_2$ over a greater proportion of the integration period (discussed below).

Formatted: Subscript

The CRDS uses a laser-based spectroscopic technique that measures the individual carbon isotopologues (^{12}C and ^{13}C) of CO_2 at ~ 1 Hz and converts to standard $\delta^{13}\text{C}$ (‰) notation (referenced to Vienna PeeDee Belemnite). When the instrument is set in the CO_2 isotope only operating mode as used in this experiment ([the CRDS can also simultaneously determine the carbon stable isotope ratio of methane](#)), the guaranteed precision of the instrument by the manufacturer is 0.05 % for the CO_2 concentration (ppm) and 0.12 ‰ for $\delta^{13}\text{C}$ (1σ , 5 min average) spanning 380 to 2000 ppm. $\delta^{13}\text{C-DIC}$ was determined using the $\delta^{13}\text{C}$ values of the extracted CO_2 measured during the integration period (see Determination of $\delta^{13}\text{C-DIC}$).

The coupling of the two instruments was achieved by simply linking the outlet of the AIRICA's NDIR analyser with the inlet of the CRDS using polyethylene lined Bev-A-Line® IV (1/8" ID, 1/4" OD) tubing (Fig. 1). A vent ensured no pressure build up at the inlet of the CRDS or backpressure on the AIRICA as the gas flow rate for the AIRICA varied from 70 to 300 ml min^{-1} (discussed below), while the CRDS has a flow rate of $\sim 35 \text{ ml min}^{-1}$. An additional drying agent (magnesium perchlorate) was used to dry the gas stream prior to entering the CRDS to minimise any potential artefacts in isotope values introduced by uncertainties in the manufacturers in-built water vapour corrections (Nara et al., 2012). Magnesium perchlorate was used as it does not induce a delay in CO_2 response time as is the case with some other desiccants (e.g. Drierite) (Webb et al., 2016).

To maximise precision and accuracy, DIC and $\delta^{13}\text{C-DIC}$ were determined from separate injections. The measurement parameters were customised for each analysis such that the integration period for DIC and $\delta^{13}\text{C-DIC}$ were 100 s and 310 s respectively. Therefore, in order to achieve autonomous measurement of DIC and $\delta^{13}\text{C-DIC}$, a computer script using AutoIt (Carvalho, 2017) was developed to autonomously modify the AIRICA's operating parameters at pre-determined time intervals without the need for an operator (the computer script is supplied as supplementary information). The script was sequenced so that a single measurement cycle consisted of the AIRICA system acidifying three aliquots of sample. The first aliquot was used to flush the system, the second aliquot was to determine DIC concentration, and the third aliquot was to determine $\delta^{13}\text{C-DIC}$.

DIC. The system was flushed with carrier gas between each aliquot to remove the excess CO₂ and return to carrier gas concentrations. The cycle was then repeated, achieving a DIC and δ¹³C-DIC measurement, on average, every ~ 16 minutes (refer to supplementary Figure S1 for a depiction of the typical CRDS output for a single measurement cycle).

2.3 Procedure

To determine DIC, the AIRICA's syringe pump was rinsed twice with 2100 μl of sample (filled and emptied at 300 μl s⁻¹) with the first rinse going directly to waste and the second rinse wasted via the stripper (Fig. 1). The syringe pump then drew 2000 μl of sample at 200 μl s⁻¹ which was then injected at 80 μl s⁻¹ into the stripper to which two drops of 10 % H₃PO₄ had been added. With a carrier gas flow rate through the stripper set a 300 ml min⁻¹, DIC concentrations were determined from integrating the CO₂ mixing ratio signal in the LICOR during an integration period of 100 s. The system was then flushed with carrier gas at 150 ml min⁻¹ to purge the liberated CO₂ from the system and return to carrier gas values prior to δ¹³C-DIC sampling. Sampling volume for δ¹³C-DIC was the same as for DIC, however, to obtain a longer integration period the following AIRICA parameters were adjusted: the rate the sample was injected from the syringe pump to the stripper (i.e. injection rate) was reduced to 15 μl s⁻¹ (from 80 μl s⁻¹); the carrier gas flow rate through the stripper was reduced to 70 ml min⁻¹ (from 300 ml min⁻¹); and the integration period was increased to 310 s (from 100 s). δ¹³C-DIC was determined from the δ¹³C-CO₂ data measured at ~ 1Hz during the integration period (discussed below). After the sampling for δ¹³C-DIC was completed, the cycle was restarted autonomously using the custom AutoIt script.

2.4 Determination of δ¹³C-DIC

The δ¹³C-CO₂ of the gas stream is a function of the carrier gas and that of the liberated CO₂ from the acidified sample (Eq. 1):

$$\delta^{13}\text{C}_{\text{total}} = (\delta^{13}\text{C}_{\text{carrier}} \times \text{frac CO}_{2\text{carrier}}) + (\delta^{13}\text{C}_{\text{sample}} \times \text{frac CO}_{2\text{sample}}) \quad (1)$$

whereby

$$\text{frac CO}_{2\text{carrier}} = \text{CO}_{2\text{carrier}} / \text{CO}_{2\text{total}}$$

$$\text{frac CO}_{2\text{sample}} = \text{CO}_{2\text{sample}} / \text{CO}_{2\text{total}}$$

$$\text{CO}_{2\text{sample}} = \text{CO}_{2\text{total}} - \text{CO}_{2\text{carrier}}$$

where δ¹³C_{total} is the δ¹³C-CO₂ of the measured gas stream CO₂ (‰); δ¹³C_{carrier} is the δ¹³C-CO₂ of the carrier gas CO₂ (‰); CO_{2carrier} is the ¹²⁺¹³CO₂ concentration of the carrier gas (ppm); δ¹³C_{sample} is the δ¹³C-CO₂ of the acidified sample (‰); CO_{2sample} is the ¹²⁺¹³CO₂ concentration of the acidified sample (ppm); and CO_{2total} is the ¹²⁺¹³CO₂ concentration of the measured gas stream (ppm).

The δ¹³C-CO₂ values of CO₂ concentrations less than 400 ppm were excluded due to the guaranteed specifications of the instrument spanning 380 to 2000 ppm. Of the remaining δ¹³C-CO₂ values, a mass balance was then used (to account for the δ¹³C value of the carrier gas) to determine a sample δ¹³C-CO₂ (i.e. δ¹³C_{sample}) value based on each measured CO₂ concentration (Eq. 2):

$$\delta^{13}\text{C}_{\text{sample}} = [(\delta^{13}\text{C}_{\text{total}} \times \text{CO}_{2\text{total}}) - (\delta^{13}\text{C}_{\text{carrier}} \times \text{CO}_{2\text{carrier}})] / (\text{CO}_{2\text{total}} - \text{CO}_{2\text{carrier}}) \quad (2)$$

Five iterations of outlier removal were conducted on the ~ 1 Hz $\delta^{13}\text{C}_{\text{sample}}$ values, with removal of values with an absolute difference (versus the mean of all $\delta^{13}\text{C}_{\text{sample}}$ values for the sample) greater than two times the standard deviation of the sample. The remaining $\delta^{13}\text{C}_{\text{sample}}$ values were then averaged to determine the final $\delta^{13}\text{C}$ -DIC value of the sample. All analysis was undertaken using Matlab (The Mathworks Inc., Natick, MA, USA) (see supplementary information for script).

2.5 Evaluation of precision and accuracy

$\delta^{13}\text{C}$ -DIC standards were made using Na_2CO_3 for the isotopically heavy standard (-3.2 ± 0.1 ‰) and K_2CO_3 for the depleted standard (-26.8 ± 0.1 ‰) with both solids verified by IRMS using the international reference materials NBS-19 and LSVEC. The Na_2CO_3 solid was used to make a set of five standard solutions ranging from ~ 500 to ~ 3600 $\mu\text{mol kg}^{-1}$ and one standard solution was made using the K_2CO_3 solid (~ 2000 $\mu\text{mol kg}^{-1}$).

[All standards were made by dissolving carbonate solids in ultra-pure water \(18.2 Milli-Q®\)](#). Precision was evaluated based on the standard deviation of at least six replicate measurements for each standard. Accuracy was tested by comparing AIRICA-CRDS $\delta^{13}\text{C}$ -DIC values to IRMS measured values from discrete samples collected during the bloom experiment (below). Both the precision measurements and bloom experiments were undertaken in a temperature-controlled laboratory with temperature ranging < 2 °C over the course of the experiments.

2.6 Algal bloom experiment

An algal bloom experiment was conducted to test the response of the method (Fig. 1) over an ~ 8 day period. Seawater (salinity 35.69 ppt) was collected from a nearby beach ($28^\circ 49' 22.01''\text{S}$, $153^\circ 36' 23.48''\text{E}$) the morning the experiment commenced (19/01/2016). The water was enriched with 64 $\mu\text{mol l}^{-1}$ each of nitrate (NO_3^-) and orthosilicate (SiO_4^{4-}), and 4 $\mu\text{mol l}^{-1}$ of orthophosphate (PO_4^{3-}). In order to counteract the impact of the SiO_4^{4-} addition on total alkalinity, 128 $\mu\text{mol l}^{-1}$ of hydrochloric acid (HCl) was added. The mesocosm was incubated under high pressure sodium bulbs (400W Phillips Son T Agro) at ~ 200 $\mu\text{mol m}^{-2} \text{s}^{-1}$ for 18 hrs per day (12:00 am to 6:00 am). The surface of the incubation vessel was covered with a transparent sheet of plastic film to inhibit evaporation and CO_2 exchange with the atmosphere allowing for an interpretation of the results in terms of a closed system. Macroalgae (*Ulva sp.*) and an additional dose of nutrients, were added to the sample water on the 25/1/16 (10:00 am) to further enhance biological activity. To achieve unattended sampling, incubated water was continuously recirculated through a sealed Schott bottle (250 ml) at ~ 1 l min^{-1} , from where the AIRICA's high precision syringe pump drew the sample (Fig. 1). DIC and $\delta^{13}\text{C}$ -DIC were sampled autonomously according to the procedure outlined above. In order to evaluate the accuracy of the AIRICA-CRDS method, 19 discrete samples for $\delta^{13}\text{C}$ -DIC were collected throughout the bloom experiment for IRMS analysis. The samples were generally collected at the start and end of the light period from the return line of the recirculating system into 40 ml pre-combusted borosilicate vials, closed without headspace by Teflon-lined septa screw caps, poisoned with 50 μl of saturated HgCl_2 solution and stored at ~ 4 °C in the dark until analysis (within a week). The samples were also analysed for $\delta^{13}\text{C}$ -DOC to determine the isotopic composition of the carbon pool available for microbial respiration. Samples were analysed using an OI Aurora 1030W TOC analyser interfaced to a Thermo Delta V^{Plus} Isotope Ratio Mass Spectrometer (IRMS) (Maher and Eyre, 2011).

Precision of $\delta^{13}\text{C}$ -DIC and $\delta^{13}\text{C}$ -DOC IRMS measurements were $\pm 0.1\text{‰}$ and $\pm 0.3\text{‰}$ respectively. Samples for DOC concentration were analysed using a Shimadzu (TOC-VCPH) analyser. Particulate organic carbon (POC, mostly representing phytoplankton) was sampled at the end of the experiment by filtering 150 ml of the incubated water through pre-combusted GF/F filters and dried ($60\text{ }^\circ\text{C}$) before analysis. Macroalgae was sampled at the end of the experiment, dried ($60\text{ }^\circ\text{C}$) and ground prior to analysis. The $\delta^{13}\text{C}$ values of the macroalgae and the POC were measured in triplicate samples using a Thermo Flash EA coupled to a Delta V^{plus} IRMS ($\pm 0.1\text{‰}$). All $\delta^{13}\text{C}$ values are reported based on the VPDB scale.

3 Results and discussion

3.1 Precision

The AIRICA-CRDS system exhibited a relatively small but detectable concentration effect on measured $\delta^{13}\text{C}$ -DIC with an increase of 0.19‰ observed from $1000\text{ }\mu\text{mol kg}^{-1}$ to $3600\text{ }\mu\text{mol kg}^{-1}$ (Fig. 2A). It is unclear if this effect is an artefact of the system or if it can be explained by ingassing of isotopically lighter atmospheric CO_2 (due to the high total alkalinity to DIC ratio of the standards) during the making of standards. CO_2 ingassing would have a larger effect on lower concentration standards (making them more depleted) than higher concentration standards, which follows the pattern observed here (Fig. 2A). Similarly, Bass et al. (2012) reported a concentration effect of $< 0.2\text{‰}$ increase from $1000\text{ }\mu\text{mol kg}^{-1}$ to $2100\text{ }\mu\text{mol kg}^{-1}$ and did not correct $\delta^{13}\text{C}$ -DIC values as the observed effect was within the precision of internal calibration standards.

The AIRICA-CRDS method had decreasing $\delta^{13}\text{C}$ -DIC uncertainty with higher DIC concentrations (Fig. 2B). Standard deviations of the isotopically heavy standards decreased from $\pm 0.17\text{‰}$ at $\sim 1000\text{ }\mu\text{mol kg}^{-1}$ ($n=6$) to $\pm 0.07\text{‰}$ at $\sim 3600\text{ }\mu\text{mol kg}^{-1}$ ($n=8$), however, below $1000\text{ }\mu\text{mol kg}^{-1}$ standard deviations were relatively high ($\pm 0.63\text{‰}$ at $500\text{ }\mu\text{mol kg}^{-1}$, $n=6$). For the isotopically lighter standard, the uncertainty was $\pm 0.17\text{‰}$ at a DIC concentration of $\sim 2000\text{ }\mu\text{mol kg}^{-1}$ (Supplementary Table 1). Bass et al. (2012) also reported decreasing uncertainty with increasing concentrations of DIC. Their membrane based equilibration system attained standard deviations $< \pm 0.2\text{‰}$ for concentrations above $360\text{ }\mu\text{mol kg}^{-1}$ using a sample volume of 350 mL and an equilibration time of 720 s. In comparison, AIRICA-CRDS achieved $< \pm 0.2\text{‰}$ uncertainty at $\sim 1000\text{ }\mu\text{mol kg}^{-1}$ on a sample volume of 2 mL and an integration time of 310 s.

To achieve the manufacturer guaranteed specifications of $\pm 0.12\text{‰}$ $\delta^{13}\text{C}$ - CO_2 , CO_2 concentrations in the gas stream, which is a sum of the CO_2 in the carrier gas and the liberated CO_2 from the acidified sample, should be between 380 to 2000 ppm. The concentration of the liberated CO_2 is a function of the sample size, the injection rate, and the gas flow rate, each of which can be independently adjusted by the user through the AIRICA software. For $\delta^{13}\text{C}$ -DIC measurements, the 2 ml of sample was injected into the stripper at $15\text{ }\mu\text{l s}^{-1}$ and extracted with a carrier gas flow rate of 70 ml min^{-1} (achieving a total measurement time of 310 s), resulting in the AIRICA-CRDS achieving an average precision of $0.14 \pm 0.04\text{‰}$ ($n = 84$) for all standards above $1000\text{ }\mu\text{mol kg}^{-1}$. While we optimised the system for coastal and oceanic DIC concentrations, if sampling low DIC concentrations (i.e. $< 1000\text{ }\mu\text{mol kg}^{-1}$), similarly precise $\delta^{13}\text{C}$ -DIC values may be achievable if, for example, a larger syringe volume is used to increase sample size. This ability for customisation adds to the functionality of the AIRICA-CRDS system. In comparison to the AIRICA-CRDS reported here, a worldwide proficiency test of

$\delta^{13}\text{C}$ -DIC analysis found laboratory precision ranged from 0.1 to 0.5 ‰ depending on different methodologies (Van Geldern et al., 2013). However, the inter-laboratory results revealed average standard deviations of ± 0.45 ‰ and ± 0.47 ‰ for $\delta^{13}\text{C}$ -DIC values for lake water and seawater measurements respectively.

3.2 Accuracy

Accuracy of the AIRICA-CRDS $\delta^{13}\text{C}$ -DIC was determined by direct comparison with IRMS measurements collected simultaneously during the algal bloom experiment (Fig. 3). The average difference in measured $\delta^{13}\text{C}$ values between methods was 0.1 ± 0.06 ‰ which is similar to the accuracy of the IRMS (0.1 ‰). This robust relationship was based on DIC concentrations ranging from $1986 \mu\text{mol kg}^{-1}$ to $2232 \mu\text{mol kg}^{-1}$ (average $2129 \mu\text{mol kg}^{-1}$) during the dynamic bloom experiment. This demonstrates that the automated AIRICA-CRDS system described here attains similar accuracy to IRMS $\delta^{13}\text{C}$ -DIC measurements at typical coastal and oceanic DIC concentrations.

3.3 Bloom experiment

The performance of the AIRICA-CRDS to characterise changes in $\delta^{13}\text{C}$ -DIC values and DIC concentrations in the marine environment is demonstrated by the algal bloom experiment (Fig. 4A). A total of 664 DIC concentrations and 661 $\delta^{13}\text{C}$ -DIC values were autonomously measured during the ~ 8 day incubation. Concentrations of DIC ranged from 1965 to $2253 \mu\text{mol kg}^{-1}$ and $\delta^{13}\text{C}$ -DIC ranged from 0.96 ‰ to -3.61 ‰.

The AIRICA-CRDS method captured a temporally inverse relationship between $\delta^{13}\text{C}$ -DIC values and DIC concentrations throughout the algal bloom experiment. During the first 3 days respiration was the dominant metabolic process releasing isotopically lighter DIC (originating from organic matter). Respiration increased the pool of DIC from ~ 1995 to ~ $2230 \mu\text{mol kg}^{-1}$ and simultaneously ~~depleted~~lowered $\delta^{13}\text{C}$ -DIC from ~ 0.7 ‰ to ~ -2.7 ‰. After 3 days diel cycling (light-dark) of DIC and $\delta^{13}\text{C}$ -DIC commenced, likely due to the time lag associated with primary producer biomass increase after the initial addition of nutrients. During daylight hours, photosynthetic production preferentially consumed the isotopically lighter $^{12}\text{CO}_2$ component of the DIC pool, decreasing DIC concentrations and ~~enriching~~increasing $\delta^{13}\text{C}$ -DIC values. Conversely, during the dark hours, respiration increased DIC concentrations and decreased $\delta^{13}\text{C}$ -DIC values. Over the course of days 4, 5 and 6, overall net production drew down the DIC pool. On day 7 no dark incubation occurred resulting in a large photosynthetically-driven decrease in the DIC concentration from $2164 \mu\text{mol kg}^{-1}$ to $1965 \mu\text{mol kg}^{-1}$ and an ~~enrichment~~increase of $\delta^{13}\text{C}$ -DIC from ~ -3.1 ‰ to ~ -1.7 ‰. [Similar diel variations were observed for DIC and \$\delta^{13}\text{C}\$ -DIC in a mesocosm coral reef metabolism experiment](#) (Bass et al., 2012).

3.4 Insights from high resolution DIC and $\delta^{13}\text{C}$ -DIC measurements

The AIRICA-CRDS's high resolution measurements of $\delta^{13}\text{C}$ -DIC can provide insights into drivers of DIC in aquatic environments. To illustrate a potential application of the AIRICA-CRDS approach, Keeling plots are used to interpret carbon sources during a simulated algal bloom experiment. Keeling plots (Keeling, 1958) visualize a simple two component mixing model and are commonly used to interpret sources of added carbon in aquatic, terrestrial and atmospheric sciences ([see Pataki et al. \(2003\) for details on underlying assumptions and types of regression models available](#)). Using a ~~m~~Model II regression ([which assumes significant errors in the measurement of both variables](#)), the y-intercept of the regression between the inverse of DIC concentration

(1/DIC) and $\delta^{13}\text{C}$ -DIC estimates the isotopic composition of the carbon source. The approach has been used to determine the isotopic composition of the DIC source in various settings including freshwater lakes (Karlsson et al., 2007), coral reefs (Carvalho et al., 2015), mangroves (Maher et al., 2013a) and groundwaters (Porowska, 2015).

The $\delta^{13}\text{C}$ -DIC source/sink values were estimated by Keeling plots for each linear increase (respiration) and decrease (production) in DIC concentrations during the simulated algal bloom based on 5-point averages of measured DIC and $\delta^{13}\text{C}$ -DIC (Fig. S2). The uncertainty in the intercept (i.e. the $\delta^{13}\text{C}$ -DIC source value) is dependent on the rate of change in DIC concentration during the dark incubation period (see Pataki et al. (2003) and references therein for regression formulations). Uncertainty decreased as the absolute change in DIC increased, achieving $< 2\%$ uncertainty when the change in DIC was greater than $\sim 40\ \mu\text{mol kg}^{-1}$ (Fig. 5). It is noted that the intercept uncertainty is much higher than the uncertainty for each $\delta^{13}\text{C}$ -DIC and DIC value ($\pm 0.14\%$ and ± 1.5 to $2\ \mu\text{mol kg}^{-1}$ respectively). A Keeling plots based on DIC concentrations during dark incubation periods over the first three incubation days (Fig. S2a), when respiration was the dominant process (Table 1, Fig. S2a,b,e), produced a $\delta^{13}\text{C}$ -DIC intercept values of $-27.8 \pm 1.2\%$ which is similar to that of terrestrial C3 vegetation (Smith and Epstein, 1971) ($-25.9 \pm 1.8\%$, $-29.3 \pm 0.4\%$ and $-33.3 \pm 0.6\%$). In contrast, the $\delta^{13}\text{C}$ -DIC intercept value for the final dark incubation of $-17.4 \pm 0.9\%$ (Table 1, Fig. S2b,f) is similar to that of marine organic matter (OM). Furthermore, $\delta^{13}\text{C}$ -DIC intercept values determined from linear decreases in DIC (i.e. photosynthetic carbon fixation) are also similar to marine OM (Fry and Sherr, 1989) ($-17.4 \pm 2\%$ and $-19.0 \pm 0.3\%$, Table 1, Fig. S2d,e). Thus, results suggest a distinct shift in the source of DIC during the course of the experiment, from terrestrially derived OM present in the sampled coastal seawater to marine derived OM at the end. This is likely due to a shift towards a dominance of marine organic matter toward the end of the experiment as a result of the algal bloom and the added macroalgae (added on day 6, Fig. 4).

The DOC results support our interpretation of a shift in the DIC source. DOC concentrations increased from $88\ \mu\text{mol kg}^{-1}$ at the beginning of the experiment to $364\ \mu\text{mol kg}^{-1}$ at the end. $\delta^{13}\text{C}$ -DOC values became more depleted for decreased during the first 3 days of the experiment before becoming more enriched increasing during the final ~ 2 days. Keeling plot intercepts based on DOC concentrations for the initial ~ 3 day period ($-31.8 \pm 1.5\%$) and final ~ 2 day period ($-17.6 \pm 2\%$) suggests a distinct shift in the carbon source contributing to the DOC pool from a terrestrially derived DOC source to a marine source. This is consistent with the shift observed in the DIC pool. The IRMS $\delta^{13}\text{C}$ -POC results for phytoplankton (-25.7%) and macroalgae (i.e. *Ulva sp.*, -10.1%) suggests a similar contribution of both sources to the final $\delta^{13}\text{C}$ -DOC intercept value of -17.6% and the $\delta^{13}\text{C}$ -DIC value of -17.384% . The AIRICA-CRDS system could similarly be used to characterise the importance of various other processes, such as, the relative importance of organic matter respiration versus carbonate dissolution as a source of DIC from coastal systems (Carvalho et al., 2015) and the importance of allochthonous versus autochthonous organic matter for supporting bacterial productivity (Guillemette et al., 2013).

Formatted: Superscript

Formatted: Superscript

Formatted: Font: Italic

4 Comments

The utility of the AIRICA-CRDS method for autonomous, high resolution measurements of DIC and $\delta^{13}\text{C}$ -DIC in a laboratory configuration has been demonstrated. Yet, the simple system also has the capacity for field deployment. Both of the commercially available instruments (coupled without any modifications to their hardware) have been used in field-based studies. CRDS have been deployed in a range of environmental settings including large research vessels (Bass et al., 2014b;Becker et al., 2012), vehicles (Maher et al., 2014), and small boats (Maher et al., 2015). Determination of DIC based on the NDIR gas analysis method has been used to conduct continuous shipboard measurements (Friederich et al., 2002;Hiscock and Millero, 2005) and the AIRICA system has been deployed on research vessels to determine concentrations of DIC from discrete samples (Balch et al., 2016;Bates et al., 2014;Bates et al., 2013). Assuming access to an appropriate power source and suitable environmental conditions to house the instruments, the AIRICA-CRDS system has potential to be deployed in the field, [however, further testing is required to test this capability.](#)

The AIRICA-CRDS is an alternative system that enables autonomous, high resolution measurements of DIC and $\delta^{13}\text{C}$ -DIC with precision and accuracy comparable to traditional IRMS techniques. In the described configuration, the system achieved a sampling resolution of 16 mins, with a DIC precision of $\pm 1.5\text{-}2 \mu\text{mol kg}^{-1}$ and $\delta^{13}\text{C}$ -DIC precision of $\pm 0.14 \text{‰}$ for concentrations spanning 1000 to 3600 $\mu\text{mol kg}^{-1}$. A change in DIC concentrations of $\sim 40 \mu\text{mol kg}^{-1}$ was sufficient to obtain a precision of $< 2 \text{‰}$ in source interpretations based on Keeling plots. Whilst we optimized the system for typical estuarine/marine DIC concentrations, the system has the potential to be optimised for other environments through changes to the syringe size, sample volume and injection speed. This ability for customisation adds to the functionality of the AIRICA-CRDS system, offering the potential to explore complex carbonate systems question across a range of aquatic settings.

Author contribution

D. T. Maher, K. G. Schulz and I. R. Santos designed the study. D. T. Maher, K. G. Schulz and M. Call conducted the experiments. M. C. Carvalho developed the AutoIT script and analysed all discrete samples. K. G. Schulz developed the Matlab Scripts. M. Call prepared the manuscript with contributions from all authors.

The authors declare that they have no conflict of interest.

Acknowledgements

We acknowledge funding from the Australian Research Council through grants DE140101733, DE150100581, LE120100156. Kai G. Schulz is the recipient of an Australian Research Council Future Fellowship (FT120100384).

Supporting information available

Detailed supporting information is available. The supporting information includes the AutoIt script, Matlab script and supplementary figures and tables.

References

- Baer, D. S., Paul, J. B., Gupta, M., and O'Keefe, A.: Sensitive absorption measurements in the near-infrared region using off-axis integrated-cavity-output spectroscopy, *Applied Physics B*, 75, 261-265, 10.1007/s00340-002-0971-z, 2002.
- Balch, W. M., Bates, N. R., Lam, P. J., Twining, B. S., Rosengard, S. Z., Bowler, B. C., Drapeau, D. T., Garley, R., Lubelczyk, L. C., Mitchell, C., and Rauschenberg, S.: Factors regulating the Great Calcite Belt in the Southern Ocean and its biogeochemical significance, *Global Biogeochemical Cycles*, 30, 1124-1144, 10.1002/2016GB005414, 2016.
- Bandstra, L., Hales, B., and Takahashi, T.: High-frequency measurements of total CO₂: Method development and first oceanographic observations, *Marine Chemistry*, 100, 24-38, <http://dx.doi.org/10.1016/j.marchem.2005.10.009>, 2006.
- Bass, A. M., Bird, M. I., Munksgaard, N. C., and Wurster, C. M.: ISO-CADICA: Isotopic – continuous, automated dissolved inorganic carbon analyser, *Rapid Communications in Mass Spectrometry*, 26, 639-644, 10.1002/rcm.6143, 2012.
- Bass, A. M., O'Grady, D., Berkin, C., Leblanc, M., Tweed, S., Nelson, P. N., and Bird, M. I.: High diurnal variation in dissolved inorganic C, $\delta^{13}\text{C}$ values and surface efflux of CO₂ in a seasonal tropical floodplain, *Environmental Chemistry Letters*, 11, 399-405, 10.1007/s10311-013-0421-7, 2013.
- Bass, A. M., Munksgaard, N. C., Leblanc, M., Tweed, S., and Bird, M. I.: Contrasting carbon export dynamics of human impacted and pristine tropical catchments in response to a short-lived discharge event, *Hydrological Processes*, 28, 1835-1843, 10.1002/hyp.9716, 2014a.
- Bass, A. M., Munksgaard, N. C., O'Grady, D., Williams, M. J. M., Bostock, H. C., Rintoul, S. R., and Bird, M. I.: Continuous shipboard measurements of oceanic $\delta^{18}\text{O}$, δD and $\delta^{13}\text{C}_{\text{DIC}}$ along a transect from New Zealand to Antarctica using cavity ring-down isotope spectrometry, *Journal of Marine Systems*, 137, 21-27, 10.1016/j.jmarsys.2014.04.003, 2014b.
- Bates, N. R., Orchowaska, M. I., Garley, R., and Mathis, J. T.: Summertime calcium carbonate undersaturation in shelf waters of the western Arctic Ocean: how biological processes exacerbate the impact of ocean acidification, *Biogeosciences*, 10, 5281-5309, 10.5194/bg-10-5281-2013, 2013.
- Bates, N. R., Garley, R., Frey, K. E., Shake, K. L., and Mathis, J. T.: Sea-ice melt CO₂-carbonate chemistry in the western Arctic Ocean: meltwater contributions to air-sea CO₂ gas exchange, mixed-layer properties and rates of net community production under sea ice, *Biogeosciences*, 11, 6769-6789, 10.5194/bg-11-6769-2014, 2014.
- Becker, M., Andersen, N., Fiedler, B., Fietzek, P., Körtzinger, A., Steinhoff, T., and Friedrichs, G.: Using cavity ringdown spectroscopy for continuous monitoring of $\delta^{13}\text{C}(\text{CO}_2)$ and $f\text{CO}_2$ in the surface ocean, *Limnology and Oceanography: Methods*, 10, 752-766, 10.4319/lom.2012.10.752, 2012.
- Becker, M., Andersen, N., Erlenkeuser, H., Humphreys, T., Tanhua, T., and Körtzinger, A.: An Internally Consistent Dataset of $\delta^{13}\text{C}$ -DIC in the North Atlantic Ocean - NAC13v1, *Earth Syst. Sci. Data Discuss.*, 2016, 1-18, 10.5194/essd-2016-7, 2016.
- Berryman, E. M., Marshall, J. D., Rahn, T., Cook, S. P., and Litvak, M.: Adaptation of continuous-flow cavity ring-down spectroscopy for batch analysis of $\delta^{13}\text{C}$ of CO₂ and comparison with isotope ratio mass spectrometry, *Rapid communications in mass spectrometry : RCM*, 25, 2355-2360, 2011.
- Byrne, R. H.: Measuring Ocean Acidification: New Technology for a New Era of Ocean Chemistry, *Environmental Science & Technology*, 48, 5352-5360, 10.1021/es405819p, 2014.
- Carvalho, M. C., Santos, I. R., Maher, D. T., Cyronak, T., McMahon, A., Schulz, K. G., and Eyre, B. D.: Drivers of carbon isotopic fractionation in a coral reef lagoon: Predominance of demand over supply, *Geochimica et Cosmochimica Acta*, 153, 105-115, <http://dx.doi.org/10.1016/j.gca.2015.01.012>, 2015.

Carvalho, M. C.: Practical Laboratory Automation Made Easy with AutoIt, Wiley-VCH, Weinheim, 290 pp., 2017.

Crosson, E. R.: A cavity ring-down analyzer for measuring atmospheric levels of methane, carbon dioxide, and water vapor, *Applied Physics B*, 92, 403-408, 10.1007/s00340-008-3135-y, 2008.

Fassbender, A. J., Sabine, C. L., Lawrence-Slavas, N., De Carlo, E. H., Meinig, C., and Maenner Jones, S.: Robust Sensor for Extended Autonomous Measurements of Surface Ocean Dissolved Inorganic Carbon, *Environmental Science & Technology*, 49, 3628-3635, 10.1021/es5047183, 2015.

Friederich, G. E., Walz, P. M., Burczynski, M. G., and Chavez, F. P.: Inorganic carbon in the central California upwelling system during the 1997–1999 El Niño–La Niña event, *Progress in Oceanography*, 54, 185-203, [http://dx.doi.org/10.1016/S0079-6611\(02\)00049-6](http://dx.doi.org/10.1016/S0079-6611(02)00049-6), 2002.

Fry, B., and Sherr, E. B.: $\delta^{13}\text{C}$ Measurements as Indicators of Carbon Flow in Marine and Freshwater Ecosystems, in: *Stable Isotopes in Ecological Research*, edited by: Rundel, P. W., Ehleringer, J. R., and Nagy, K. A., Springer New York, New York, NY, 196-229, 1989.

Gattuso, J.-P., and Hansson, L.: Ocean acidification: background and history, in: *Ocean Acidification*, edited by: Hansson, L., and Gattuso, J.-P., Oxford University Press, 1-20, 2011.

Goyet, C., and Snover, A. K.: High-accuracy measurements of total dissolved inorganic carbon in the ocean: comparison of alternate detection methods, *Marine Chemistry*, 44, 235-242, 10.1016/0304-4203(93)90205-3, 1993.

Guillemette, F., McCallister, S. L., and del Giorgio, P. A.: Differentiating the degradation dynamics of algal and terrestrial carbon within complex natural dissolved organic carbon in temperate lakes, *Journal of Geophysical Research: Biogeosciences*, 118, 963-973, 10.1002/jgrg.20077, 2013.

Hiscock, W. T., and Millero, F. J.: Nutrient and carbon parameters during the Southern Ocean iron experiment (SOFEX), *Deep Sea Research Part I: Oceanographic Research Papers*, 52, 2086-2108, <http://dx.doi.org/10.1016/j.dsr.2005.06.010>, 2005.

Huang, K., Cassar, N., Jonsson, B., Cai, W.-j., and Bender, M. L.: An Ultrahigh Precision, High-Frequency Dissolved Inorganic Carbon Analyzer Based on Dual Isotope Dilution and Cavity Ring-Down Spectroscopy, *Environmental Science & Technology*, 49, 8602-8610, 10.1021/acs.est.5b01036, 2015.

Karlsson, J., Jansson, M., and Jonsson, A.: Respiration of allochthonous organic carbon in unproductive forest lakes determined by the Keeling plot method, *Limnology and Oceanography*, 52, 603-608, 2007.

Keeling, C. D.: The concentration and isotopic abundances of atmospheric carbon dioxide in rural areas, *Geochimica et Cosmochimica Acta*, 13, 322-334, [http://dx.doi.org/10.1016/0016-7037\(58\)90033-4](http://dx.doi.org/10.1016/0016-7037(58)90033-4), 1958.

Le Quéré, C., Moriarty, R., Andrew, R. M., Canadell, J. G., Sitch, S., Korsbakken, J. I., Friedlingstein, P., Peters, G. P., Andres, R. J., Boden, T. A., Houghton, R. A., House, J. I., Keeling, R. F., Tans, P., Arneeth, A., Bakker, D. C. E., Barbero, L., Bopp, L., Chang, J., Chevallier, F., Chini, L. P., Ciais, P., Fader, M., Feely, R. A., Gkritzalis, T., Harris, I., Hauck, J., Ilyina, T., Jain, A. K., Kato, E., Kitidis, V., Klein Goldewijk, K., Koven, C., Landschützer, P., Lauvset, S. K., Lefèvre, N., Lenton, A., Lima, I. D., Metzl, N., Millero, F., Munro, D. R., Murata, A., S. Nabel, J. E. M., Nakaoka, S., Nojiri, Y., O'Brien, K., Olsen, A., Ono, T., Pérez, F. F., Pfeil, B., Pierrot, D., Poulter, B., Rehder, G., Rödenbeck, C., Saito, S., Schuster, U., Schwinger, J., Séférian, R., Steinhoff, T., Stocker, B. D., Sutton, A. J., Takahashi, T., Tilbrook, B., Van Der Laan-Luijkx, I. T., Van Der Werf, G. R., Van Heuven, S., Vandemark, D., Viovy, N., Wiltshire, A., Zaehle, S., and Zeng, N.: Global Carbon Budget 2015, *Earth System Science Data*, 7, 349-396, 10.5194/essd-7-349-2015, 2015.

Li, X., and Liu, W.: Effect of preservation on the delta ^{13}C value of dissolved inorganic carbon in different types of water samples, *Isotopes in environmental and health studies*, 47, 379-389, 10.1080/10256016.2011.598934, 2011.

Liu, X., Byrne, R. H., Adornato, L., Yates, K. K., Kaltenbacher, E., Ding, X., and Yang, B.: In Situ Spectrophotometric Measurement of Dissolved Inorganic Carbon in Seawater, *Environmental Science & Technology*, 47, 11106-11114, 10.1021/es4014807, 2013.

Maher, D., and Eyre, B. D.: Insights into estuarine benthic dissolved organic carbon (DOC) dynamics using $\delta^{13}\text{C}$ -DOC values, phospholipid fatty acids and dissolved organic nutrient fluxes, *Geochimica et Cosmochimica Acta*, 75, 1889-1902, 10.1016/j.gca.2011.01.007, 2011.

Maher, D. T., Santos, I. R., Golsby-Smith, L., Gleeson, J., and Eyre, B. D.: Groundwater-derived dissolved inorganic and organic carbon exports from a mangrove tidal creek: The missing mangrove carbon sink?, *Limnology and Oceanography*, 58, 475-488, 10.4319/lo.2013.58.2.0475, 2013a.

Maher, D. T., Santos, I. R., Leuven, J. R. F. W., Oakes, J. M., Erler, D. V., Carvalho, M. C., and Eyre, B. D.: Novel Use of Cavity Ring-down Spectroscopy to Investigate Aquatic Carbon Cycling from Microbial to Ecosystem Scales, *Environmental Science & Technology*, 47, 12938-12945, 10.1021/es4027776, 2013b.

Maher, D. T., Santos, I. R., and Tait, D. R.: Mapping Methane and Carbon Dioxide Concentrations and $\delta^{13}\text{C}$ Values in the Atmosphere of Two Australian Coal Seam Gas Fields, *Water, Air, & Soil Pollution*, 225, 2216, 10.1007/s11270-014-2216-2, 2014.

Maher, D. T., Cowley, K., Santos, I. R., Macklin, P., and Eyre, B. D.: Methane and carbon dioxide dynamics in a subtropical estuary over a diel cycle: Insights from automated in situ radioactive and stable isotope measurements, *Marine Chemistry*, 168, 69-79, 10.1016/j.marchem.2014.10.017, 2015.

Martz, T. R., Daly, K. L., Byrne, R. H., Stillman, J. H., and Turk, D.: Technology for ocean acidification research: Needs and availability, *Oceanography*, 28, 40-47, 10.5670/oceanog.2015.30, 2015.

Midwood, A. J., and Millard, P.: Challenges in measuring the $\delta^{13}\text{C}$ of the soil surface CO_2 efflux, *Rapid Communications in Mass Spectrometry*, 25, 232-242, 10.1002/rcm.4857, 2011.

Nara, H., Tanimoto, H., Tohjima, Y., Mukai, H., Nojiri, Y., Katsumata, K., and Rella, C. W.: Effect of air composition (N_2 , O_2 , Ar, and H_2O) on CO_2 and CH_4 measurement by wavelength-scanned cavity ring-down spectroscopy: Calibration and measurement strategy, *Atmospheric Measurement Techniques*, 5, 2689-2701, 10.5194/amt-5-2689-2012, 2012.

Newton, J., Feely, R., Jewett, E., Williamson, P., and Mathis, J.: Global Ocean Acidification Observing Network: Requirements and Governance Plan. 60 pp, Online at: http://www.goa-on.org/docs/GOA-ON_plan_print.pdf, 2014.

O'Sullivan, D. W., and Millero, F. J.: Continual measurement of the total inorganic carbon in surface seawater, *Marine Chemistry*, 60, 75-83, 10.1016/S0304-4203(97)00079-0, 1998.

Pataki, D. E., Ehleringer, J. R., Flanagan, L. B., Yakir, D., Bowling, D. R., Still, C. J., Buchmann, N., Kaplan, J. O., and Berry, J. A.: The application and interpretation of Keeling plots in terrestrial carbon cycle research, *Global Biogeochemical Cycles*, 17, n/a-n/a, 10.1029/2001GB001850, 2003.

Porowska, D.: Determination of the origin of dissolved inorganic carbon in groundwater around a reclaimed landfill in Otwock using stable carbon isotopes, *Waste Management*, 39, 216-225, 10.1016/j.wasman.2015.01.044, 2015.

Sabine, C. L., Ducklow, H., and Hood, M.: International carbon coordination: Roger Revelle's legacy in the intergovernmental oceanographic commission, *Oceanography*, 23, 48-61, 2010.

Smith, B. N., and Epstein, S.: Two Categories of $^{13}\text{C}/^{12}\text{C}$ Ratios for Higher Plants, *Plant Physiology*, 47, 380-384, 1971.

Taipale, S. J., and Sonninen, E.: The influence of preservation method and time on the $\delta^{13}\text{C}$ value of dissolved inorganic carbon in water samples, *Rapid Commun Mass Spectrom*, 23, 2507-2510, 10.1002/rcm.4072, 2009.

Van Geldern, R., Verma, M. P., Carvalho, M. C., Grassa, F., Delgado-Huertas, A., Monvoisin, G., and Barth, J. A. C.: Stable carbon isotope analysis of dissolved inorganic carbon (DIC) and dissolved organic carbon (DOC) in natural waters - Results from a worldwide proficiency test, *Rapid Communications in Mass Spectrometry*, 27, 2099-2107, 10.1002/rcm.6665, 2013.

Vogel, F. R., Huang, L., Ernst, D., Giroux, L., Racki, S., and Worthy, D. E. J.: Evaluation of a cavity ring-down spectrometer for in situ observations of $^{13}\text{CO}_2$, *Atmos. Meas. Tech.*, 6, 301-308, 10.5194/amt-6-301-2013, 2013.

Webb, J. R., Maher, D. T., and Santos, I. R.: Automated, in situ measurements of dissolved CO_2 , CH_4 , and $\delta^{13}\text{C}$ values using cavity enhanced laser absorption spectrometry: Comparing response times of air-water equilibrators, *Limnology and Oceanography: Methods*, 14, 323-337, 10.1002/lom3.10092, 2016.

Table-Captions

Table 1. Keeling plot intercept values and standard deviations for the linear increase/decrease in DIC concentrations during the simulated algal bloom as indicated by the lower case letters in Figure 4. Intercept values are derived from the regression of 1/DIC concentrations vs. $\delta^{13}\text{C}$ -DIC values based on 5-point averages of measured DIC concentrations and $\delta^{13}\text{C}$ -DIC values (see Fig. S2).

	y-Intercept value (‰)
a	-25.92 ± 1.79
b	-29.34 ± 0.43
c	-33.29 ± 0.65
d	-17.43 ± 1.96
e	-19.05 ± 0.35
f	-17.38 ± 0.93

Figures

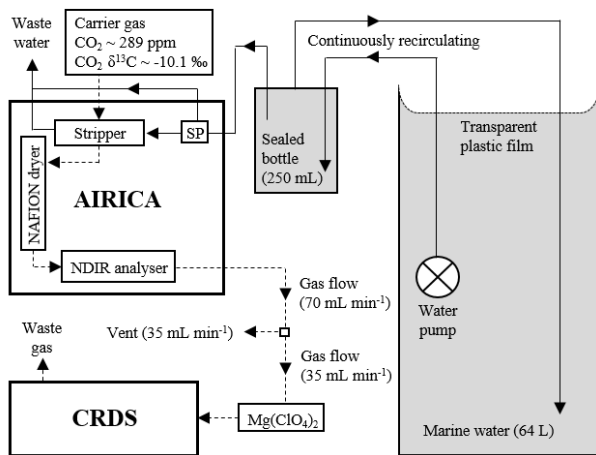


Figure 1. Schematic of the coupled Autonomous Infra Red Inorganic Carbon Analyser (AIRICA) and Cavity Ring Down Spectrometer (CRDS) set up to autonomously and continuously measure DIC concentrations and $\delta^{13}\text{C}$ -DIC values. Solid arrows indicate liquid flow and dashed arrows indicate gas flow. SP = syringe pump.

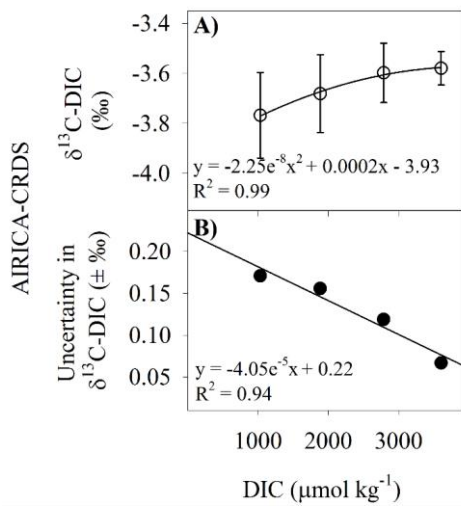


Figure 2. A) Concentration effect on $\delta^{13}\text{C-DIC}$ data produced by the AIRICA-CRDS B) Uncertainty in $\delta^{13}\text{C-DIC}$ versus DIC concentration.

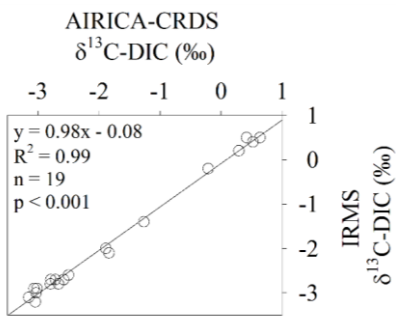
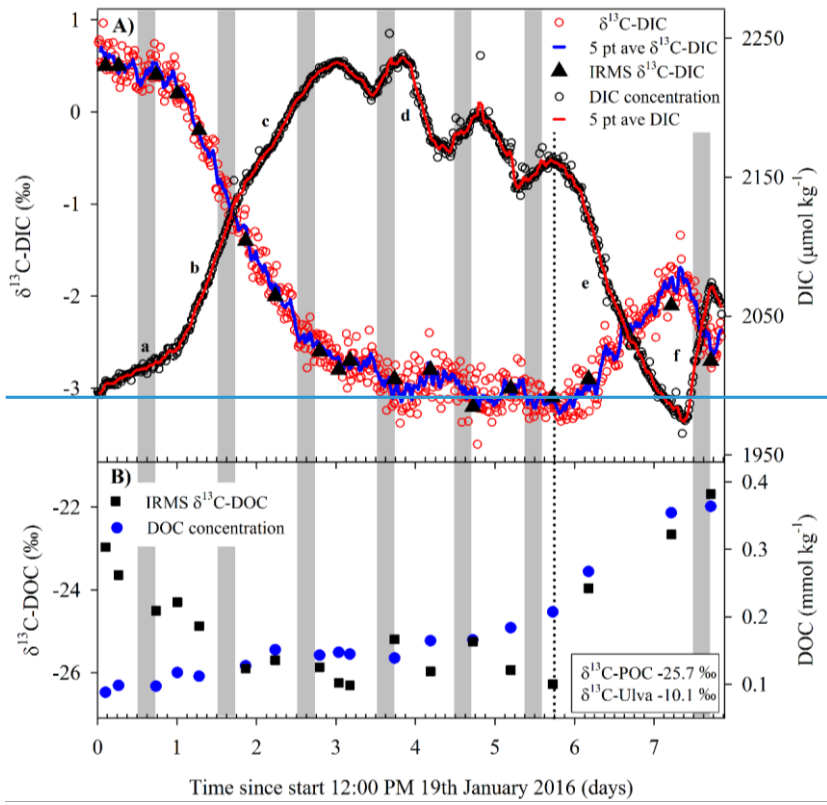


Figure 3. Comparison of AIRICA-CRDS $\delta^{13}\text{C-DIC}$ vs IRMS $\delta^{13}\text{C-DIC}$.



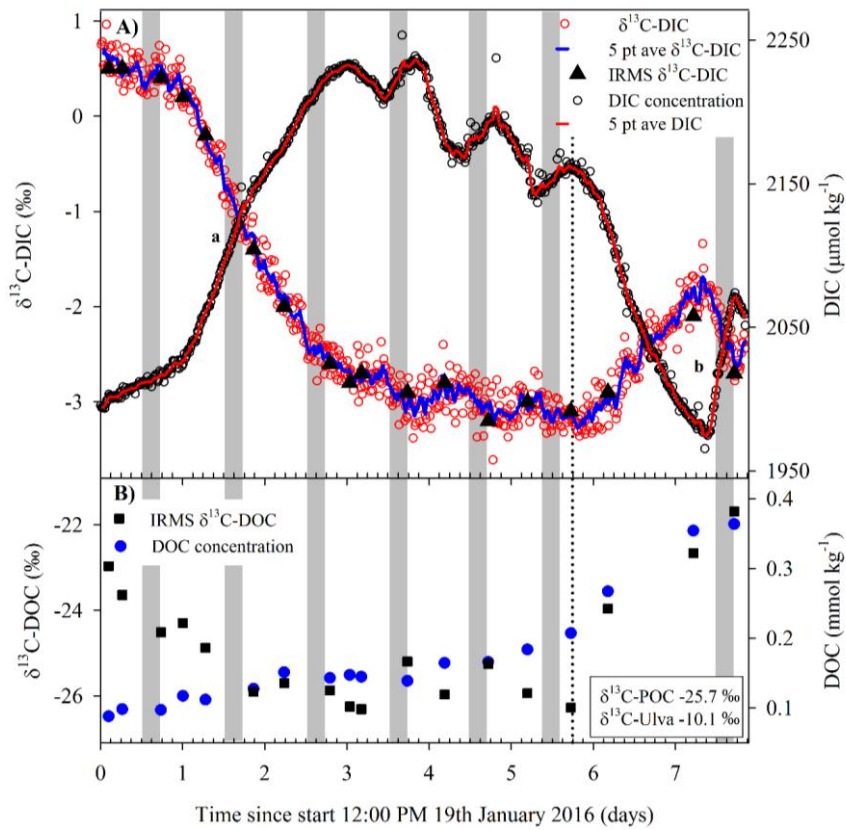


Figure 4. A) $\delta^{13}\text{C-DIC}$ values and DIC concentrations measured by the AIRICA-CRDS system during the ~ 8 day laboratory bloom experiment. Blue and red lines are 5 point averages for $\delta^{13}\text{C-DIC}$ and DIC respectively. Black triangles are discrete IRMS $\delta^{13}\text{C-DIC}$ values plotted for comparison. Shaded areas indicate dark incubations. Lower case letters indicate the sections used for Keeling plots (see Fig. S2). Dotted line is when macroalgae (*Ulva sp.*) and additional nutrients were added. B) IRMS $\delta^{13}\text{C-DOC}$ values and DOC concentrations for discrete samples. Inset box displays IRMS $\delta^{13}\text{C}$ values for POC and *Ulva sp.*

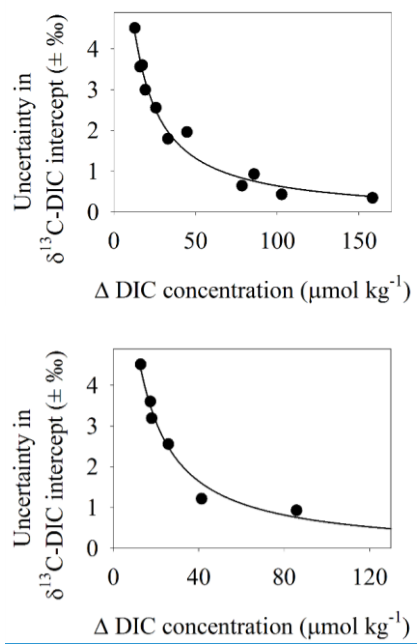


Figure 5. Relationship between Keeling intercept uncertainty and changes in DIC concentration. Higher changes in DIC resulted in lower uncertainties in Keeling plot interpretations.